依據低功率電波輻射性電機管理辦法

第十二條
※經型式認證合格之低功率射頻電機，非經許可，公司、商號或使用者均不得擅自變更頻率、加大功率或變更原設計之特性及功能。
第十四條
※低功率射頻電機之使用不得影響飛航安全及干擾合法通信；經發現有干擾現象時，應立即停用，並改善至無干擾時方得繼續使用。
-前項合法通信，指依電信法規定作業之無線電通信。
-低功率射頻電機須忍受合法通信或工業、科學及醫療用電波輻射性電機設備之干擾。

Taiwan NCC Attention!
Article 12: Without permission granted by the DGT, any company, enterprise, or user is not allowed to change frequency, enhance transmitting power or alter original characteristic as well as performance to a approved low power radio-frequency devices.

Article 14: The low power radio-frequency devices shall not influence aircraft security and interfere legal communications; If found, the user shall cease operating immediately until no interference is achieved.

The said legal communications means radio communications is operated in compliance with the Telecommunications Act.

The low power radio-frequency devices must be susceptible with the interference from legal communications or ISM radio wave radiated devices.

日康遠距健康照護
ZCON Telehealth

ADD: 高雄市前金區中正四路136號9F
9F., No.136,Zhongzheng 4th Rd.,
Qianjin Dist., Kaohsiung City 807, Taiwan
TEL: +886-7-2863100
FAX: +886-7-2862100
E-mail: service@zconhealth.com
www.zconhealth.com

日康科技有限公司 ZCON Telehealth Co.,Ltd.



i-GlucoPal
安糖寶
使用手冊

※本產品非醫療用途，數據僅供參考使用，
不可取代醫師的看診、諮詢、診斷或建議的治療。
※This product is for non-medical purposes, the data is for reference only. It could not be replaced by the physician's advice, diagnosis or recommended treatment.

i-GlucoPal
安糖寶

Available on the App Store

ANDROID APP ON Google play

安糖寶 / i-GlucoPal / 安糖宝

App商店下載

Download from **AppStore** or **Google play**

目錄 Content

03 中文說明
05 設備外觀
06 設備注意事項
07 開通帳號
08 APP功能
09 配對設備
10 開始量測:條件選擇
11 開始量測:流程教學
12 量測注意事項
13 量測結果
14 健康動態
15 量測設定
16 保健提醒
17 自校準
18 安全說明

19 English Instructions
21 Appearance
22 Notices
23 Activate Account
24 App Features
25 Bluetooth Connection
26 Start measurement: condition selection
27 Start measurement: measurement flow
28 Precautions
29 Measurement Result
30 Health Status
31 Measurement Setting
32 Health Remind
33 Self-calibration
34 Safety Instructions

35 简体中文说明
37 设备外观
38 设备注意事项
39 激活帐号
40 APP功能
41 配对设备
42 开始量测:条件选择
43 开始量测:流程教学
44 量测注意事项
45 量测结果
46 健康动态
47 量测设定
48 保健提醒
49 自校准
50 安全说明

i-GlucoPal
安糖寶

中文說明

Chinese Instructions

安糖寶操作教學影片



親愛的用戶，您好：

歡迎您成為日康遠距健康照護的貴賓用戶，非常感謝您的支持與愛護，為了讓您完全想有完善的健康服務，請先開通帳號成為日康會員。

希望在未來的日子裏，您能持續享有日康為您帶來的便利與健康照護。

若服務使用有任何問題，
歡迎您來信 service@zconhealth.com
或撥打客服專綫 +886-7-2863100
我們將竭誠為您服務。

敬祝

日日平安　天天健康

日康遠距健康照護　敬上

設備外觀




重置鍵
恢復原廠設定

工作指示燈
開機狀態亮藍燈

開機鍵
啟動電源

USB充電孔
充電連接處

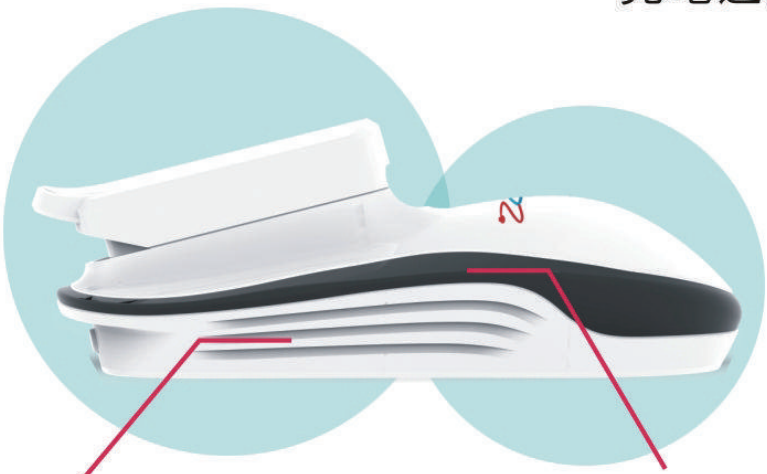

藍芽指示燈
藍芽連線時將亮藍燈

設備散熱區域

工作環境

(1) 環境溫度: 20 - 27攝氏
(2) 環境濕度: 20% - 70%
(3) 氣壓範圍: 700hPa~1060hPa
(4) 避免直接受到陽光的直接照射
(5) 避免放置於有毒物體或
易燃氣體環境下使用

電量管理

(1) 輕按開機鍵啓動安糖寶
(2) 閒置3分鐘後，將自動關機
(3) 測試完畢後，將在10秒鐘後關機
(4) 充電時請勿使用安糖寶
(5) 將電源鍵持續壓按3秒即可關機
(6) 工作額定電壓: 5V
(7) 工作額定電流: 1A

開通帳號

首次使用，請先開通您的會員帳號
請依照隨盒附贈的VIP會員卡，
選擇其一方式開通帳號。



方法 1

請上網開起開通網址：
www.zconhealth.com/devices/create
並輸入VIP卡片上的16位開通碼



方法 2

請用智慧裝置，如智慧型手機或平板，
掃描VIP卡片上的二維條碼，
即可查看並開通您的帳號。

點選左上角主選單按鈕，可顯示全部功能列表。



開始量測

→由此進入量測功能

健康動態

→觀看健康數據分析

量測紀錄

→量測數據的歷史紀錄

保健提醒

→貼心鬧鐘功能，可設定提醒

量測設定

→異常數據通知，與數據標準值設定

自校準

→App與設備自我校準設定及清除校準資料

用戶指南

→查看用戶注意事項與使用教學

量測參考標準

→參考健康數據與注意事項

配對設備

使用安糖寶量測前，請先依照以下步驟，將您的量測設備與智慧裝置連接配對。

※提醒您，請先確認您的智慧裝置已經連接網路並開啟藍芽





1. 請先打開量測設備電源和安糖寶App。

2. 在開始量測頁面，點選連結按鈕設定藍芽連線。



※iOS手機用戶請點選偵測設備

3.點選設備列表"ITON DM"或"SPPLE DM"的選項，即可連接設備。

※若無出現選項，請點選搜尋/偵測按鈕，再次搜尋。



每次用戶測試前，
請先選取最符合
當下狀況之飲食
及用藥狀態(可複選)，
再點選開始量測。

※按鈕說明

- ●清晨空腹：用戶8小時以上未進食。
- ●餐後2小時：用戶離上次進食已超過兩小時測試出真正的血糖值。
- ●測試數值依據年齡及代謝速度有不同變化

※用藥備註

1. 雙胍類主要功能是增加肝臟及肌肉對胰島素的敏感性(充分利用)。
2. 璜尿類主要是增加胰臟胰島素的分泌。
3. 抑制劑主要功能是延緩糖類在小腸的消化及吸收。
4. 糖尿病患者初期基本都是靠雙胍類控制如果三個月後複診，無法改善糖化血色素的穩定則由醫生視血糖的高低再決定要用雙胍類搭配璜尿類或類抑制劑類藥物來控制血糖。


開始量測：流程教學




1.選擇量測條件，並點選開始量測。



2.藍芽設備連接中，並檢測環境。

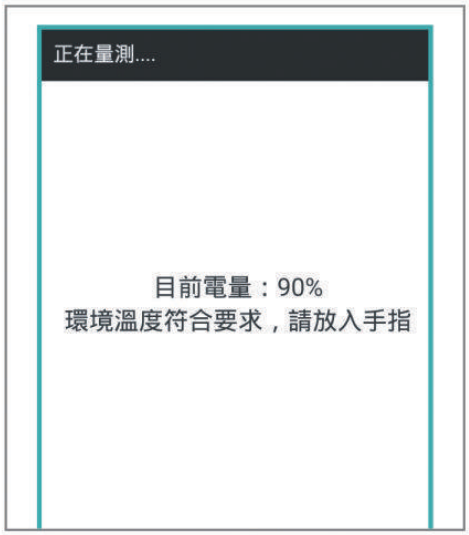

3.App會顯示請用戶放入手指，此時再放入即可。

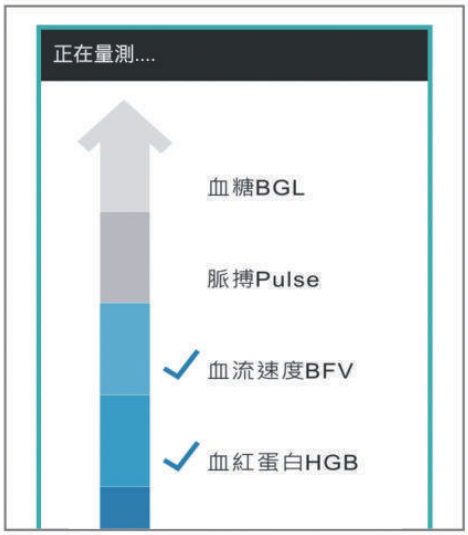

4.量測時間共60秒，請保持姿勢至量測結果出現。

※測試時手指輕放，勿重壓感測探頭，以免數據失真。

※量測過程中，用戶若遇到無法順利量測之狀況，請依照畫面提示文字進行排除。

※因Android手機型號多樣化，如軟體APP無法適應，出現掉字或無法完整顯示或無法輸入時，建議將字體大小改成中等。

使用前請注意以下事項，否則將影響測試結果



1. 請將安糖寶擺置於平面上使用



2. 檢測時請將指甲面朝上，伸至探頭底部



3. 檢測時手指需保持在 29 - 35 攝氏溫度



4. 連續檢測需間隔至少3分鐘



5. 勿使用指甲油或防曬油等隔離乳液



6. 運動過後需至少休息1小時



7. 洗澡或洗手後需至少休息30分鐘




8. 測試前請勿喝酒



9. 不能有壓迫血液的現象，
否則導致手指血流不暢

量測結果

量測數據將顯示在安糖寶App
的畫面中，並自動上傳至雲端。

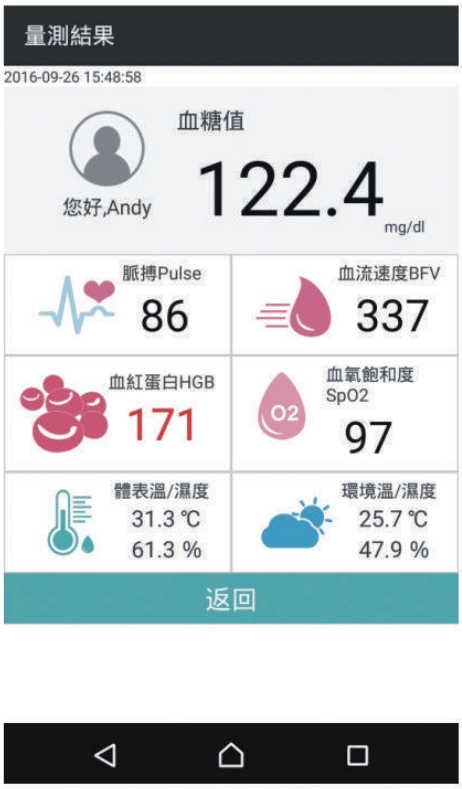




九項健康指標一目了然！
血糖、脈搏、血流速度、
血紅蛋白、血氧飽和度、
體表溫濕度、環境溫濕度。

*若有數值落在不正常的範圍，將會顯示紅字提醒用戶。

健康動態

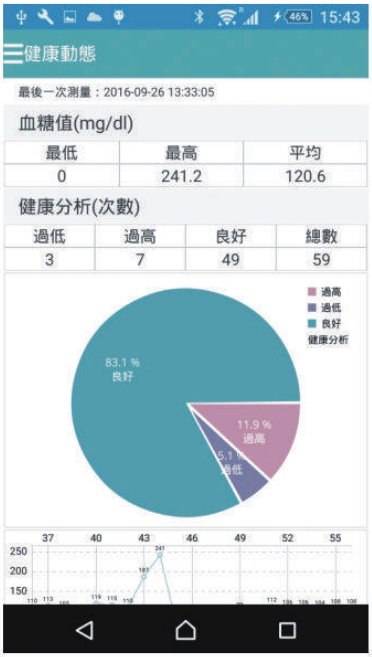

使用安糖寶健康管理，您可以隨時透過網路和APP，登入查詢您的量測記錄與健康分析。

量測紀錄

點進去可觀看更多



量測設定



您可以在此處設定
*數據異常通知和
*關懷聯絡人。

數據若有異常時，
將以E-mail寄發通知，
及時關心。



單位切換

若您所在地區，
使用的單位不同，
也可以在這裡切換
單位設定。





您可以在保健提醒中
根據您的作息，
設定提醒時間。

自校準



因人體差異，部份人群的測試結果可能會有偏差，可透過自校準拉近相似度


1.每次操作自校準時，請先選擇您最信任的血糖儀來量測血糖值。

2.把血糖生化值輸入App欄位中



3.點選開始量測。

4.量測結束即完成 1 次自校準。

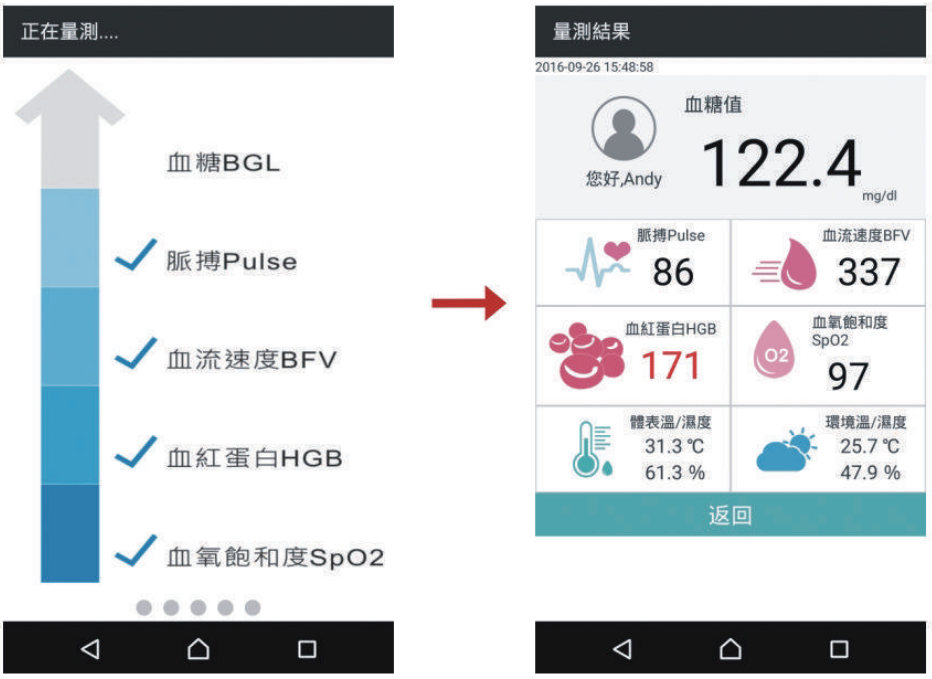

*提醒您：請於30天內完成20次清晨空腹的自校準

(01)使用前請校準本產品，確認其正常工作

(02)避免被水濺濕，若本產品被濺濕，請立刻切斷電源連絡維修人員。

(03)保持產品清潔，以軟布沾清水擰乾擦拭。整機和探頭嚴禁使用蒸氣清潔。指夾式探頭非防水，嚴禁液體流入。

(04)禁止使用高溫消毒，或使用電子射束和y 放射殺菌。

(05)確保本產品使用環境不受較強的電磁干擾源的干擾，例如無線發報機或行動電話等。

(06)在使用前，使用者必須檢查產品確保沒有明顯可能影響人身安全或儀器性能的損壞。推薦的檢查週期為每月一次或更短時間。如果發現明顯的損壞，請更換損壞零部件。

(07)在收納時，請不要將金屬物體與產品混放在一起，以免產品內置電池發生意外的短路。

(08)當產品從寒冷環境轉到溫暖、潮濕的地方，不要立即使用

(09)保持操作環境無震動、無腐蝕、無可燃物質，以及避免過高或過低的溫度和濕度。

(10)本產品必須由經過授權的合格工程師維修，請勿擅自拆開設備。

(11)雖然產品主機和探頭設計牢固，抗摔抗震。但使用中應務必小心，不能摔碰及表面劃傷。

(12)電源線需插在有兩線的插座上，不要使用不良的插座。不要隨意更換本設備的電源線。注意電源線、導管和所有電纜的放置。

(13)請將產品安裝到固定位置，避免跌落造成人員受傷或者產品損壞。

(14)本產品散熱孔嚴禁堵塞，以保證有效散熱。

(15)操作者在使用本產品監測之前，必須確認產品處於正常的工作狀態和操作環境下。

(16)定期檢查重複使用的附件是否損壞，電纜等是否連接可靠，必要時需置換並按電子廢物妥善處理已壞附件。

(17)不要在有可燃性氣體的地方使用，例如有氧氣混合的麻醉劑。

(18)請勿將電池取出，切勿將電池丟至火中以免引起爆炸。

i-GlucoPal
Cloud Health Management

English Instructions

i-GlucoPal Vedio Guide

Dear member,




You are welcome to become a VIP member of ZCON telehealth. Thank you for your support. In order to provide perfect health service, please register first to become a member. We hope in the coming days, you can continue to enjoy the convenience of our health care.

If you have any questions,
please contact us :
service@zconhealth.com
orcall our customer service hotline :
+ 886-7-2863100

We wish you have a healthy life.

Sincerely Yours
ZCON Telehealth

Appearance

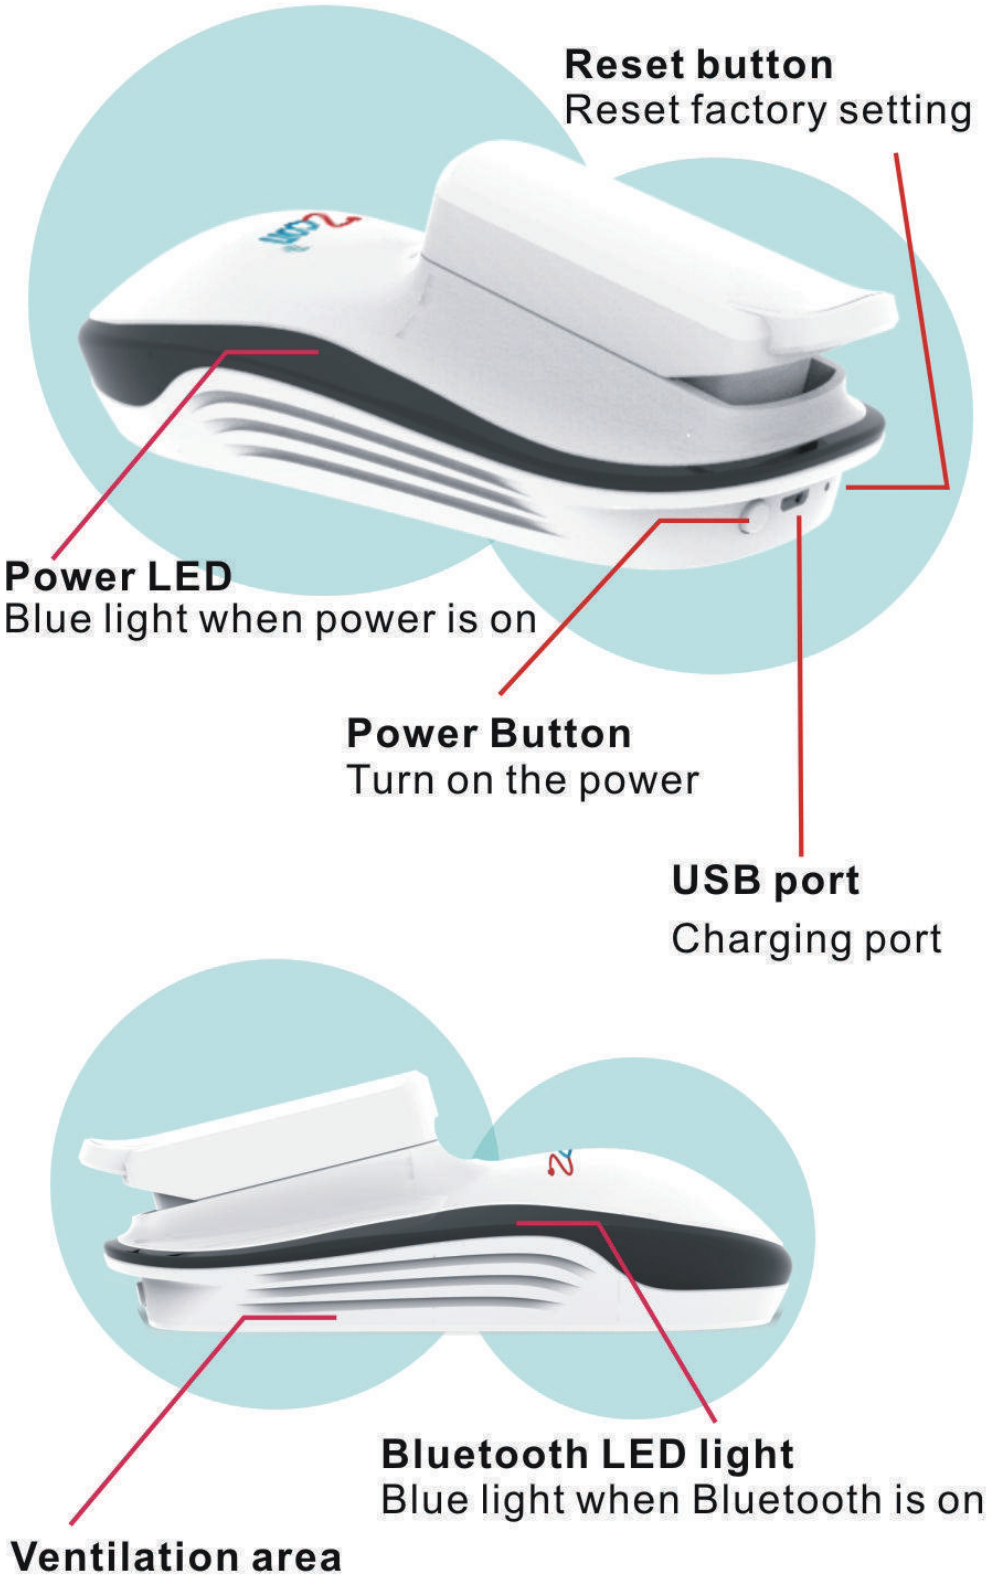
Reset button
Reset factory setting
Power LED
Blue light when power is on
Power Button
Turn on the power
USB port
Charging port
Bluetooth LED light
Blue light when Bluetooth is on
Ventilation area

Operation Conditions

(1) Temperature range: 20 - 27 degrees
(2) Humidity range: 20% - 70%
(3) Atmospheric Pressure Range: 700-1060hPa
(4) Avoid direct contact with sunlight
(5) Avoid contact with toxic or flammable gas

Power Management

(1) Press power button to switch on i-GlucoPal.
(2) i-GlucoPal will automatically shut down in 3 minutes without using.
(3) i-GlucoPal will automatically shut down in 10 seconds after testing.
(4) Testing is not allowed during charging.
(5) Press and hold power button for 3 seconds to switch off i-GlucoPal.
(6) Working Rated Voltage: 5V
(7) Working Rated Current: 1A

Activate account

For first time user,
you have to activate your account.

Please follow the instruction in the VIP card.
Choose one way to activate your account.



Method 1


Please enter this website:
www.zconhealth.com/devices/create
and enter the 16 numbers list on the card.



Method 2

Use smart devices like smartphones scan the QR code on the card, you can view and activate your account.

Tab the main menu button at the top left corner to display all the features.

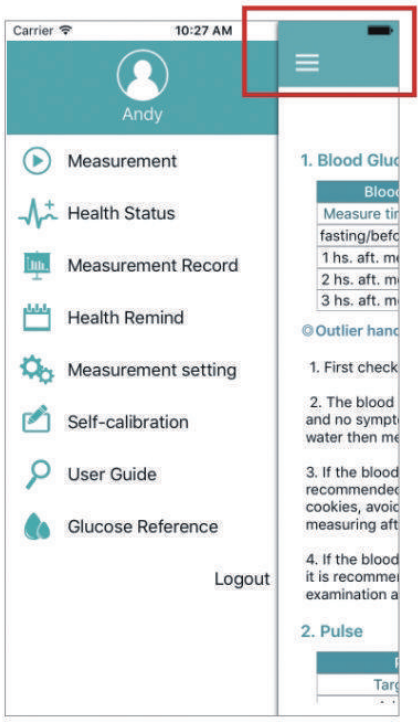

Start Measuring

→ The measurement function.

Health Dynamics

→ Watch health data analysis.

Measurement Record

→ History of measured data.

Health Reminder

→ Intimate alarm clock function, for your reminder.

Measurement Settings

→ Exception data notification and standard data setting.

Self-Calibration

→ Device self-calibration setting and clear calibration data.

User Guide

→ Check the user notes and user tutorial.

References


→Refer to health data and precautions.

Bluetooth connection

Please pair the measuring device with your smart device before measuring.




※Please make sure your device has Bluetooth turned on and connecting to the Internet.

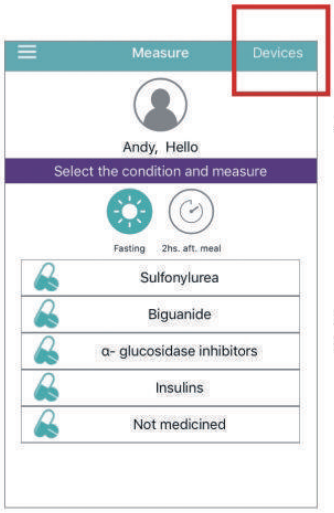

1.Please turn on the device then open the i-GlucoPal App and login.

2.Please click upper right corner button for Bluetooth setting.

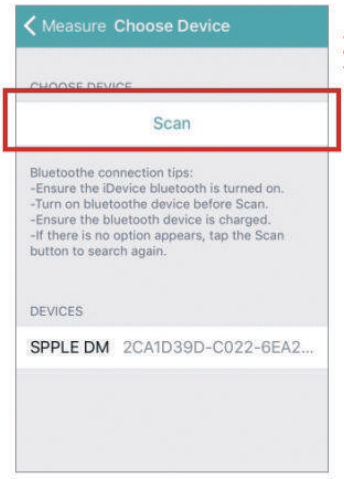


※ If you are iOS user, please tap the scan button

3. In the list of devices, you'll see "ITON DM"or “SPPLE DM” option then click to connect the device.

※ If there is no option appears, tap the button to scan again.

Start masurement:condition selection

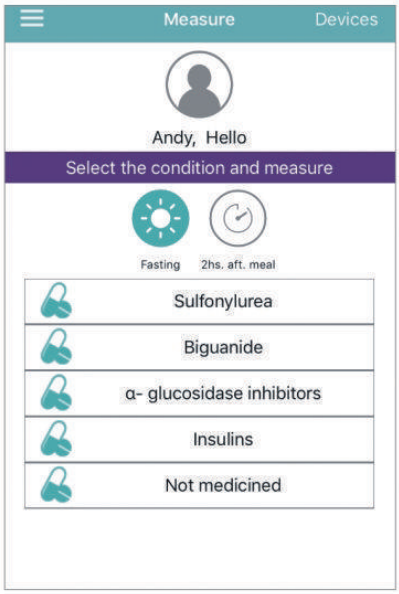

Each time before the measuring, please select the current state of meals and drug medication (multiple choice), then click the "Start Measuring"

※Button Function

●Fasting glucose: User has not eaten anything for 8 hours or more.
●2 hours have past since user's previous meal. Test to see real blood glucose value.
●Varies from age and metabolism rate.

※Track Your Health Now

1.Biguanides type: Increase the sensitivity of liver and muscles towards insulin thus less insulin is needed. Decrease the amount of sugar produced by the liver; increase the amount of sugar absorbed by muscle cells.


2.Sufonylurea type: Increase the amount of insulin Produced by pancreas.

3.Alpha Glucosidase inhibitor type: Slows down the digestion of starch in the intestine.
Pre or early diabetics take biguanides type medicines. After three months, if HbA1C is not stabilized, the doctor will prescribe sufonylurea type or alpha glucosidase inhibitor type medicines together with biguanides type medicines , according to the patient's blood glucose level.


Start Measurement: Measurement Flow




1.Please select the current state of meals and drug medication, then click the "Start Measuring".

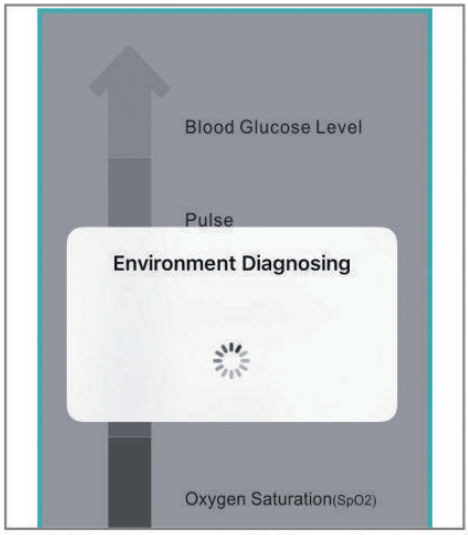

2. Please wait for detecting the environment ...

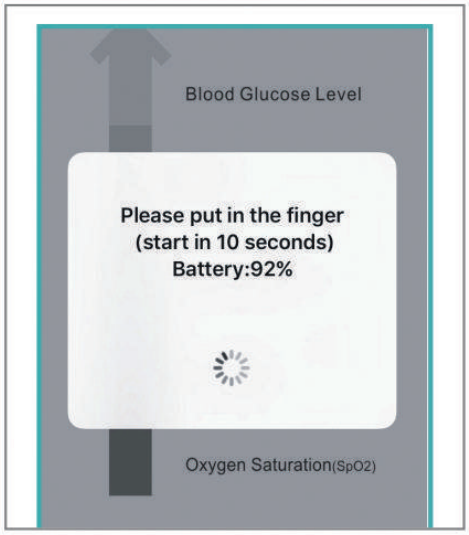

3. When the screen displays "Please insert your finger " then you can put any of your finger into the device.

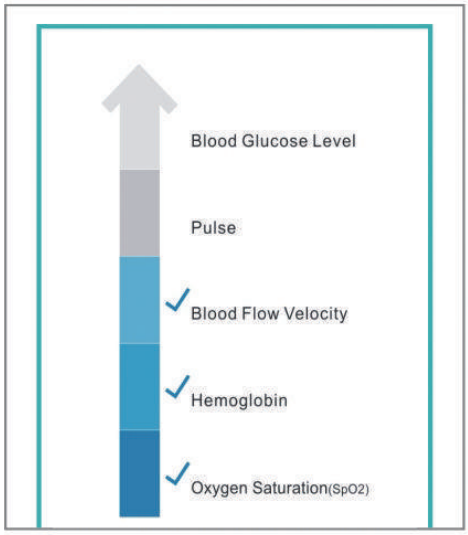

4.It will take 60 seconds for measurement. Please do not speak, and hold the position until come out the measurement results.

※Please put in finger into sensor, don t press down while testing otherwise it may affect test result.
※When have trouble of measuring, please follow the instruction to fix the problem.
※Our APP is unable to accommodate to all existing Android smart phone models, if you encounter dropping characters or unable to input text, please set your font size to medium.

» Precautions

Please be aware of the following or the test result will be affected



(1) Use i-GlucoPal only on a flat surface.



(2) Keep your nail up during the testing process.



(3) Suitable finger temperature: 29 - 35 degrees



(4) Test Interval is 3 minutes, minimum time required for heat to be fully dissipated from the sensor.



(5) Do not apply Isolation products such as nail polish and sunblock before testing.



(6) Allow cooling down after sports for at least 1 hour.



(7) Allow cooling down after bathing or washing for at least 30 minutes.



(8) Test after consuming alcohol is not allowed.



(9) Please put in finger into sensor, don't press down while testing otherwise it may affect test result.

Measurement Results

The measurement data will be displayed in the i-GlucoPal App and automatically uploaded to the cloud.




All nine health data are shown:

Blood glucose level, pulse, blood flow velocity, hemoglobin, oxygen saturation, body surface temp and humidity, environmental temp and humidity.

※It will be highlighted in red when data is outside normal range.


Health Status

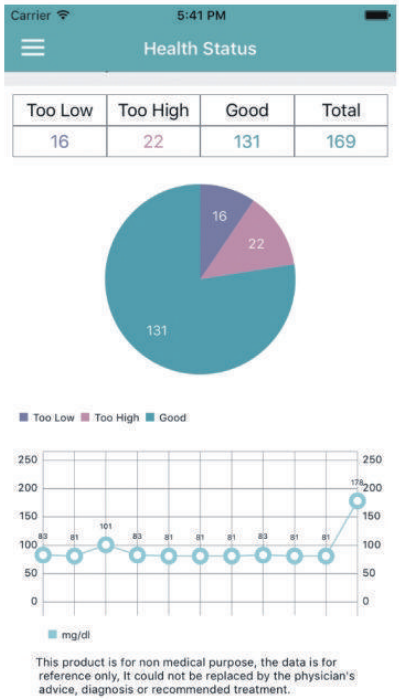


When using i-GlucoPal health management, you can use the internet and app to check your measurement records and health analysis any time.

Measurement Record

To check more data.

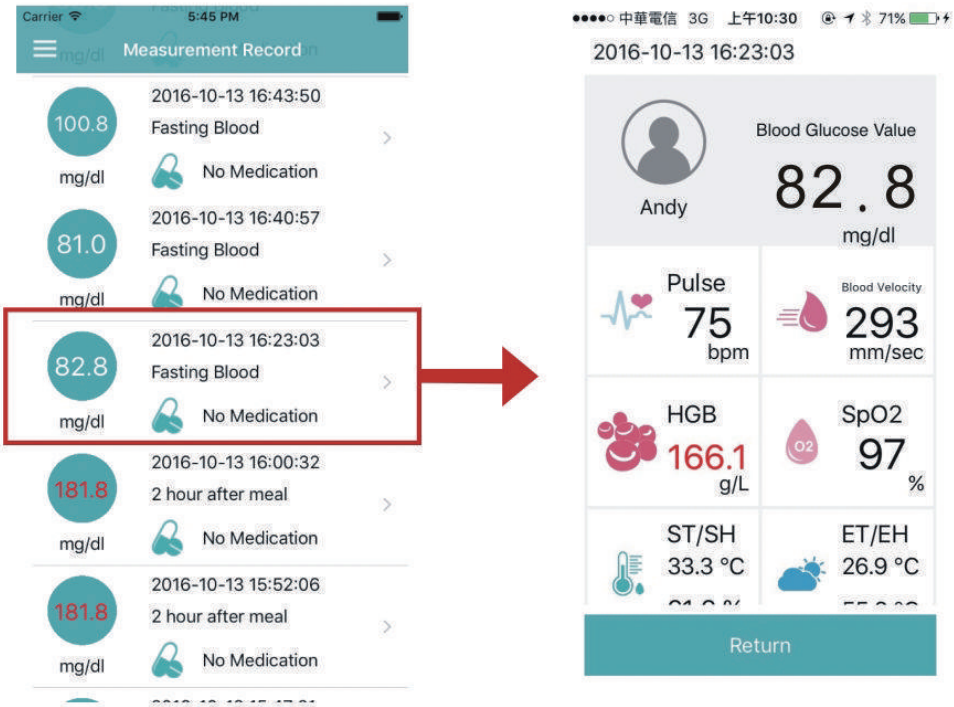


Measurement Setting

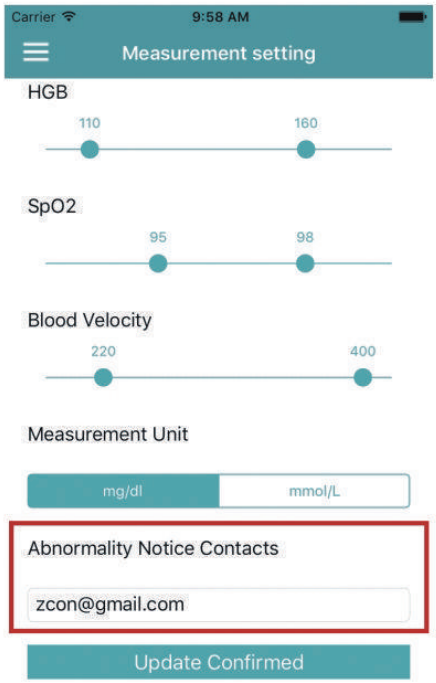

Measurement Setting


Here you can set notifications and care contact person.


When have abnormal data, we will send E-mail for notification.

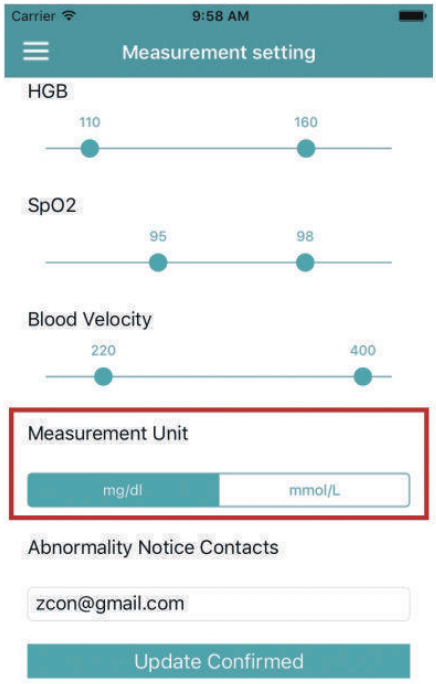

Switching Unit


You can switch unit setting depends on your area.

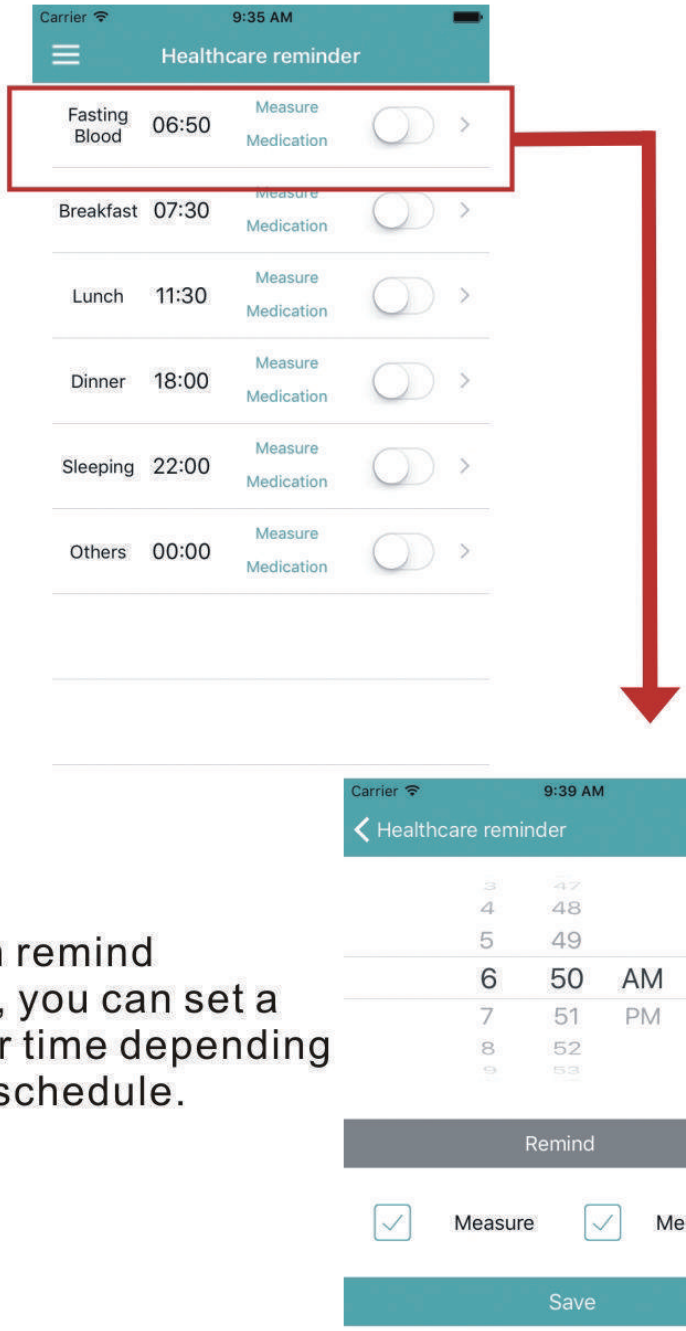

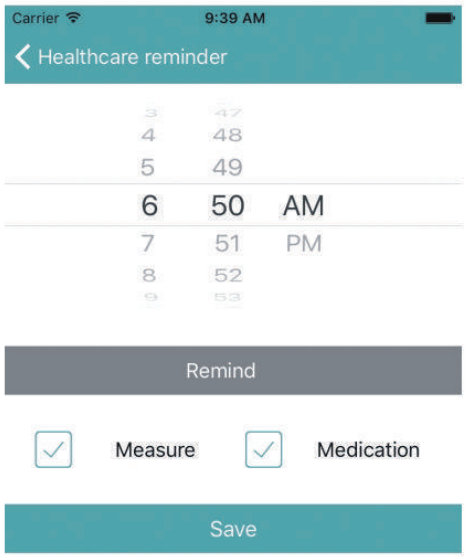

In health remind function, you can set a reminder time depending on your schedule.

Self-calibration

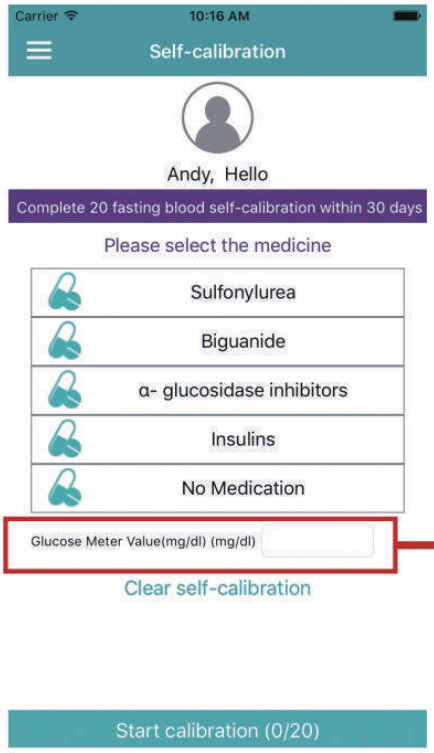


Due to differences of each body, the test results may have bias , and you can use self-calibration function to approach the similarity.

1.Each time use the self-calibration function, please select your most trusted glucose meter to measure blood glucose level.

2.Input biochemical blood sugar value to i-GlucoPal App .

3.Start measuring.

4.Finish each measuring then complete a self-calibration.

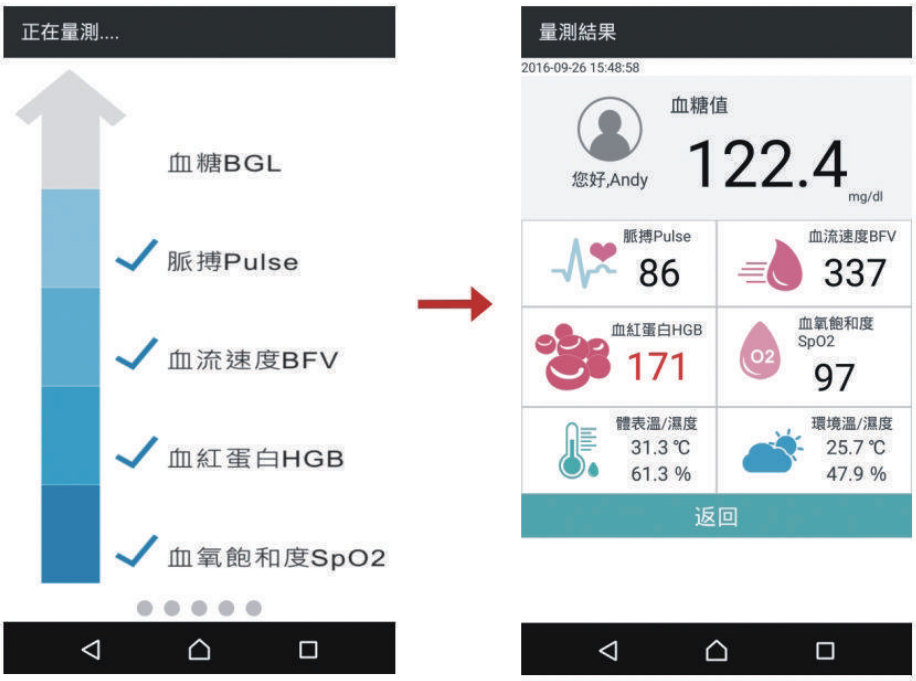

*Remind you: Please complete 20 self-calibrations of fasting in 30 days.

(1) Before use, calibrate i-GlucoPal to en sure it works normally.
(2) Protect i-GlucoPal from water. Once spattered, cut off the power supply, switch off and contact service.
(3) Keep i-GlucoPal clean. Use a soft damp cloth to clean and sterilise. DO NOT use steam to sterilise. Protect nonwaterproof finger clip probe from any liquids.
(4) DO NOT sterilise under high temperature or disinfect with electron beam or radiation.
(5) Ensure i-GlucoPal is not disturbed by strong EMI, such as from a radio transmitter or mobile phone.
(6) Before use, check any damage that may harm personal safety or affect i-GlucoPal performance. Once per month or more frequent checks are recommended. If any damage is found, replace the damaged part immediately.
(7) DO NOT store i-GlucoPal near metal objects to avoid accidental short circuiting of the inbuilt battery.
(8) DO NOT use i-GlucoPal immediately after taking it from a cold to a warmer and more humid place.
(9) Keep i-GlucoPal from vibrating, corrosive, and flammable materials. Protect from extreme temperatures and humidity.
(10) i-GlucoPal must be maintained by authorised and qualified engineers. DO NOT disassemble.
(11) Do not throw ,hit ,or scratch surface of i-GlucoPal.
(12) The power wire needs to be connected to a two-wire socket. DO NOT use a defective socket. DO NOT replace the power wire arbitrarily. Place wires, conduits, and all cables properly.
(13) Install i-GlucoPal at a fixed place to avoid injuries and damage caused by falling.
(14) DO NOT block the i-GlucoPal's ventilation to ensure effective heat dissipation.
(15) Before testing, ensure i-GlucoPal is working normally, in a suitable environment.
(16) Check and replace frequently used accessories and cables; Dispose damaged parts as electronic waste properly.
(17) DO NOT use in a place with flammable gas, such as oxygen-mixed anesthetic.
(18) DO NOT take out the battery. DO NOT throw the battery into the fire, it may explode.

i-GlucoPal
安糖宝

简体中文说明

Simplified Chinese Instructions

安糖宝操作教学影片



亲爱的用户，您好：

欢迎您成为日康远距健康照护的贵宾用户，非常感谢您的支持与爱护，为了让您完全享有完善的健康服务，请先开通账号成为日康会员。

希望在未来的日子里，您能持续享有日康为您带来的便利与健康照护。

若服务使用有任何问题，
欢迎您来信 service@zconhealth.com
或拨打客服专线 +886-7-2863100
我们将竭诚为您服务。

敬祝

日日平安　天天健康

日康远距健康照护 敬上

设备外观


重置键
恢复原厂设定
工作指示灯
开机状态亮蓝灯
开机键
启动电源
USB充电孔
充电连接处
设备散热区域
蓝芽指示灯
蓝芽联机时将亮蓝灯

工作环境

(1)环境温度: 20 - 27摄氏

(2)环境湿度: 20% - 70%

(3)气压范围: 700hPa~1060hPa

(4)避免直接受到阳光的直接照射

(5)避免放置于有毒物体或
易燃气体环境下使用

电量管理

(1)轻按开机键启动安糖宝

(2)闲置3分钟后，将自动关机

(3)测试完毕后，将在10秒钟后关机

(4)充电时请勿使用安糖宝

(5)将电源键持续压按3秒即可关机

(6)工作额定电压: 5V

(7)工作额定电流: 1A

激活帐号

首次使用，请先激活您的会员帐号

请依照随盒附赠的VIP会员卡，
选择其一方式激活帐号。



方法 1

请开启开通网址
www.zconhealth.com/devices/create

并输入VIP卡片上的16位激活码(开通码)



方法 2

请用智能装置，如智能手机或平板，
扫描卡片上的二维条码，
即可查看并激活您的帐号

点选左上角主选单按钮，可显示全部功能列表。



开始量测

→由此进入量测功能

健康动态

→观看健康数据分析

量测记录

→量测数据的历史记录

保健提醒

→贴心闹钟功能，可设定提醒

量测设定

→异常数据通知，与数据标准值设定

自校准

→App与设备自我校准设定与清除校准资料

用户指南

→查看用户注意事项与使用教学

血糖参考标准

→参考健康数据与注意事项

配对设备

使用安糖宝量测前，请先依照以下步骤，将您的量测设备与智能装置连接配对。

※提醒您，请先确认您的智能装置已经连接网路并开启蓝芽。





1.请先打开量测设备电源和安糖宝App。

2.在开始量测頁面，点选连结按钮设定蓝芽连线。



※iOS用户请先点选侦测设备

3. 点选设备列表"ITON DM"或"SPPLE DM"的选项，即可连接设备。

※若无出现选项，请点选搜寻/侦测按钮，再次搜寻。



每次用户测试前，
请先选取最符合
当下状况之饮食
及用药状态(可复选)，
再点选开始量测。



※按钮说明

●清晨空腹：用户8小时以上未进食
●餐后两小时：用户离上次进食已超过两小时测试出真正的血糖值
●测试数值依据年龄及代谢速度有不同变化

※用药备注

1. 双胍类主要功能是增加肝脏及肌肉对胰岛素的敏感性(充分利用)
2. 璜尿类主要是增加胰脏胰岛素的分泌
3. 抑制剂主要功能是延缓糖类在小肠的消化及吸收
4. 糖尿病患者初期基本都是靠双胍类控制如果三个月后复诊， 无法改善糖化血色素的稳定则由医生视血糖的高低再决定要用双胍类搭配璜尿类或 类抑制剂类药物来控制血糖

开始量测：流程教学




1.选择量测条件，并点选开始量测



2.蓝芽设备连接中，并检测环境



3.App会显示请用户放入手指，此时再放入即可。

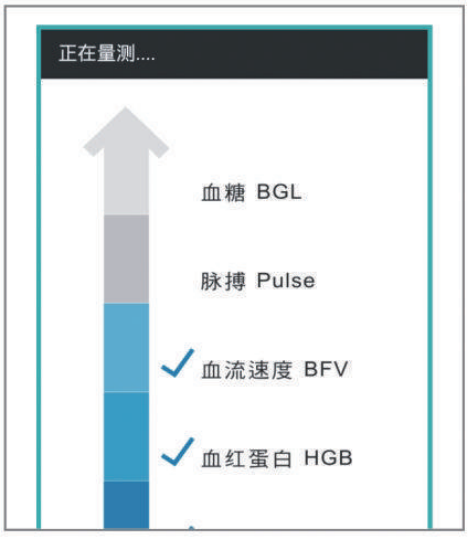

4.量测时间共60秒，请保持姿势至量测结果出现。

※测试时手指轻放，勿重压感测探头，以免数据失真。

※量测过程中，用户若遇到无法顺利量测之状况，请依照画面提示文字进行排除。

※因Android手机型号多样化，如软体App无法适应，出现掉字或无法完整显示或无法输入时，建议将字体大小改成中等。

使用前请注意以下事项，否则将影响测试结果



1. 请将安糖宝摆置于平面上使用



2. 检测时请将指甲面朝上，伸至探头底部



3. 检测时手指需保持在29 - 35摄氏温度



4. 连续检测需间隔至少3分钟



5. 勿使用指甲油或防晒油等隔离乳液



6. 运动过后需至少休息1小时



7. 洗澡或洗手后需至少休息30分钟




8. 测试前请勿喝酒



9. 不能有压迫血液的现象，
否则导致手指血流不畅

量测结果

量测数据将显示在安糖宝App的
画面中，并自动上传至云端。

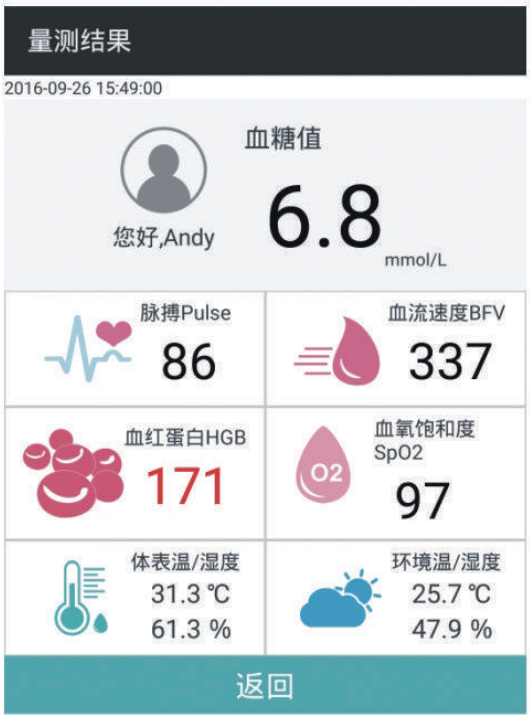




九项健康指标一目了然!
血糖、脉搏、血流速度、
血红蛋白、血氧饱和度、
体表温湿度、环境温湿度。

*若有数值落在不正常的范围，将会显示红字提醒用户

健康动态

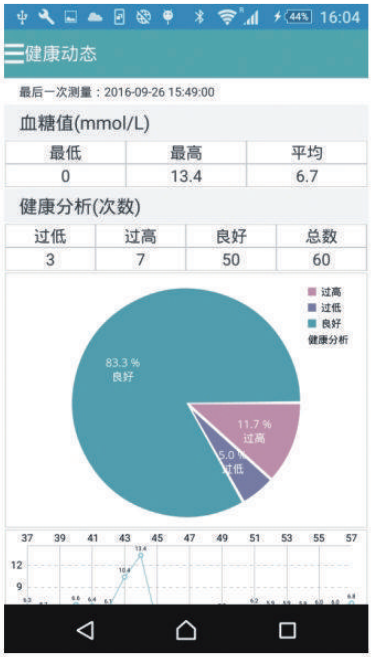

使用安糖宝健康管理，您可以随时透过网路和APP，登入查询您的量测记录与健康分析。

量测纪录

点进去可观看更多





您可以在此处设定
*数据异常通知 和
*关怀联络人

数据若有异常时，
将以E-mail寄发通知，
及时关心。



单位切换


若您所在地区，
使用的单位不同，
也可以在这里切换
单位设定。



您可以在保健提醒中
根据您的作息，
设定提醒时间



自校准

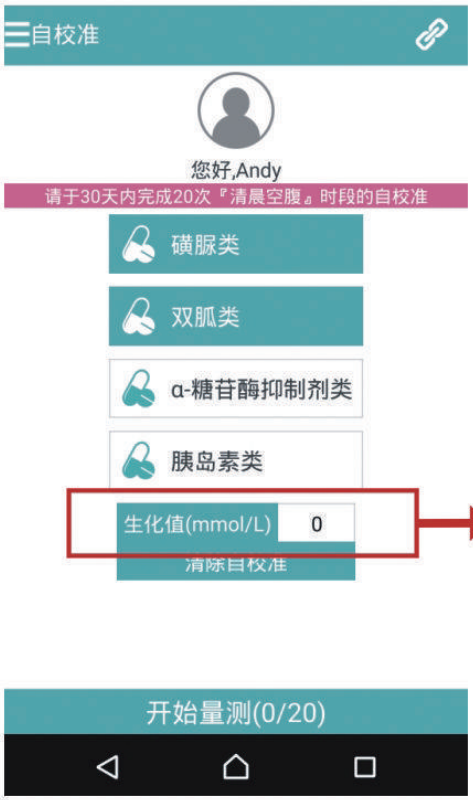


因人体差异，部份人群的测试结果可能会有偏差，可透过自校准拉近相似度。

1. 每次操作自校准时，请先选择您最信任的血糖仪来量测血糖值。

2. 把血糖生化值输入App欄位中

3.點選开始量测。

4.量测结束即完成1次自校准。

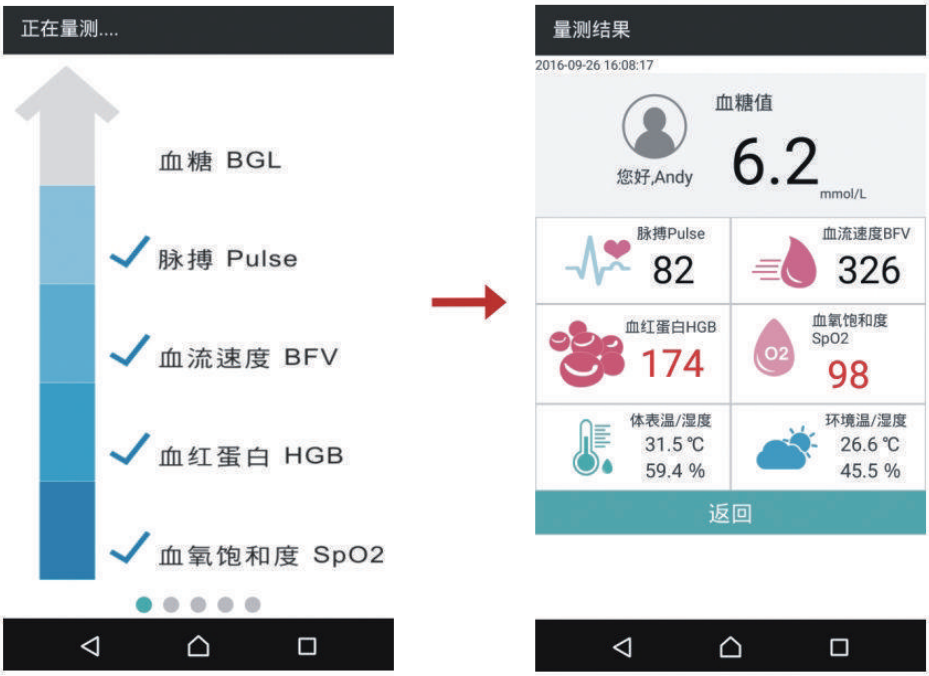

*提醒您：请于30天内完成20次清晨空腹的自校准

(1)使用前请校准本产品，确认其正常工作。

(2)避免被水溅湿，若本产品被溅湿，请立刻切断电源并连络维修人员。

(3)保持产品清洁，以软布沾清水拧干擦拭。整机和探头严禁使用蒸气清洁。指夹式探头非防水，严禁液体流入。

(4)禁止使用高温消毒，或使用电子射束和y 放射杀菌。

(5)确保本产品使用环境不受较强的电磁干扰源的干扰，例如无线发报机或移动电话等。

(6)在使用前，用户必须检查产品确保没有明显可能影响人身安全或仪器性能的损坏。推荐的检查周期为每月一次或更短时间。如果发现明显的损坏，请更换损坏零部件。

(7)在收纳时，请不要将金属物体与产品混放在一起，以免产品内置电池发生意外的短路。

(8)当产品从寒冷环境转到温暖、潮湿的地方，不要立即使用。

(9)保持操作环境无震动、无腐蚀、无可燃物质，以及避免过高或过低的温度和湿度。

(10)本产品必须由经过授权的合格工程师维修，请勿擅自拆开设备。

(11)虽然产品主机和探头设计牢固，抗摔抗震。但使用中应务必小心，不能摔碰及表面划伤。

(12)电源线需插在有两线的插座上，不要使用不良的插座。不要随意更换本设备的电源线。注意电源线、导管和所有电缆的放置。

(13)请将产品安装到固定位置，避免跌落造成人员受伤或者产品损坏。

(14)本产品散热孔严禁堵塞，以保证有效散热。

(15)操作者在使用本产品监测之前，必须确认产品处于正常的工作状态和操作环境下。

(16)定期检查重复使用的附件是否损坏，电缆等是否连接可靠，必要时需置换并按电子废物妥善处理已坏附件。

(17)不要在有可燃性气体的地方使用，例如有氧气混合的麻醉剂。

(18)请勿将电池取出，切勿将电池丢至火中，以免引起爆炸。